CRYO SYSTEM

FLARE HISTORICAL DATA - Air Lock

Back to Menu

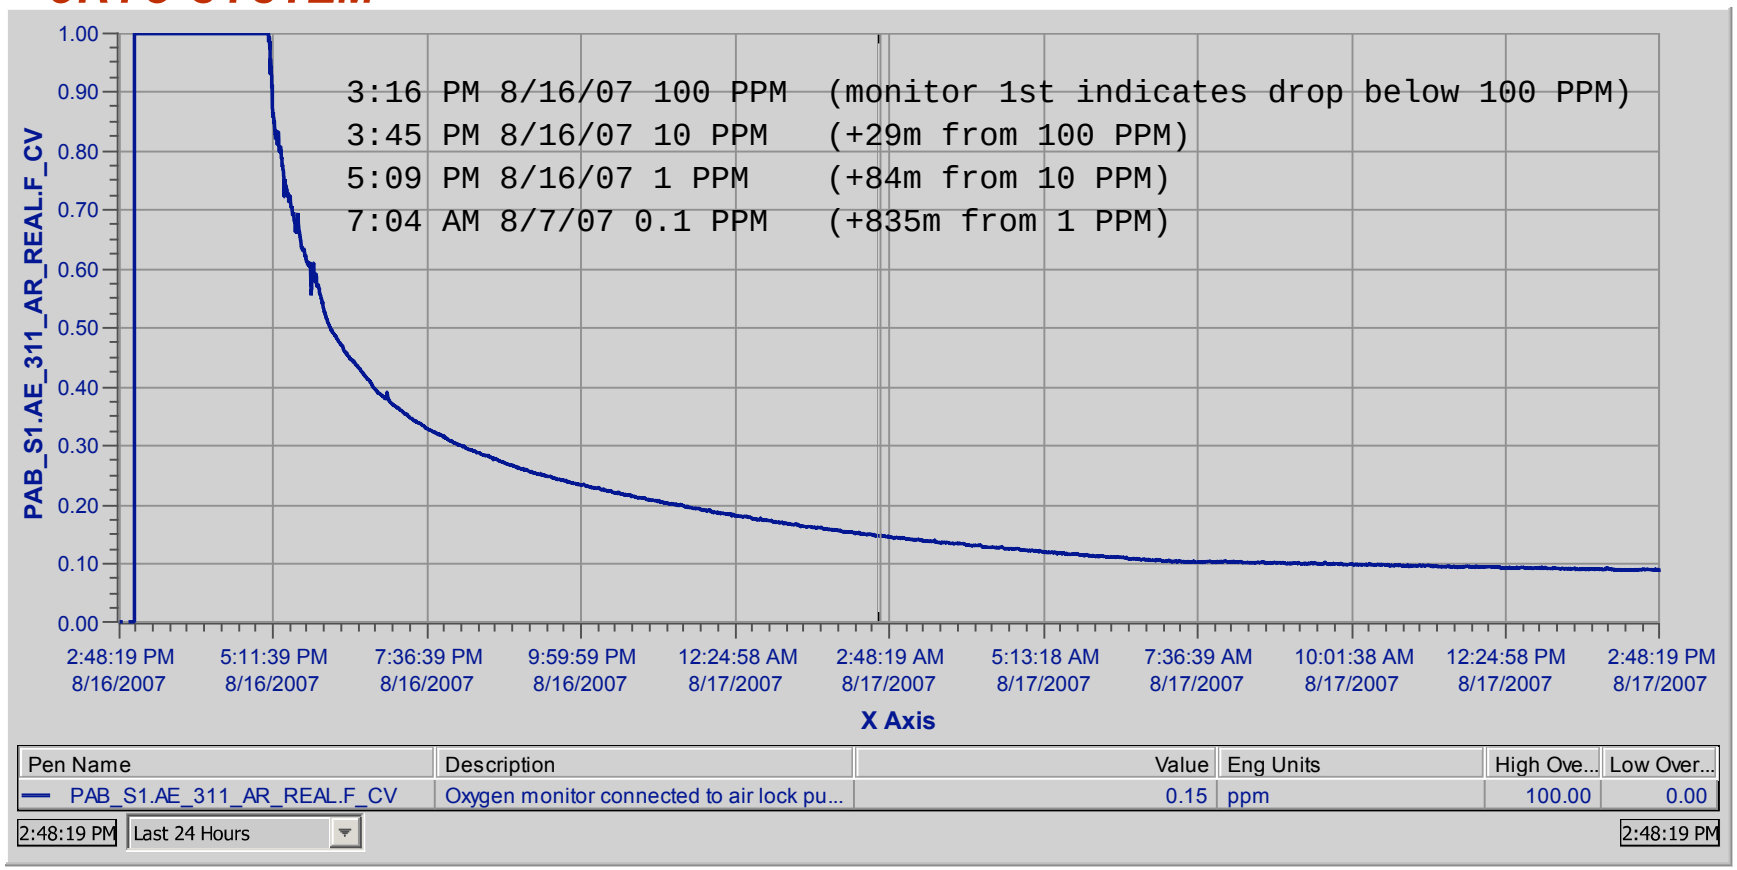

Pen Name	Description	Value	Eng Units	High Ove...	Low Over...
PAB_S1.AE_311_AR_REAL.F_CV	Oxygen monitor connected to air lock pu...	0.15	ppm	100.00	0.00

2:48:19 PM | Last 24 Hours | 2:48:19 PM

Data from materials lock purge oxygen monitor.
Boiloff from cryostat was used to purge airlock. Boiloff rate was calculated as 23.4 SCFH gas. Cryostat is at about 6.3 PSIG during this venting.