CRYO SYSTEM

FLARE HISTORICAL DATA - OXYGEN FILTER REGENERATION

Back to Menu

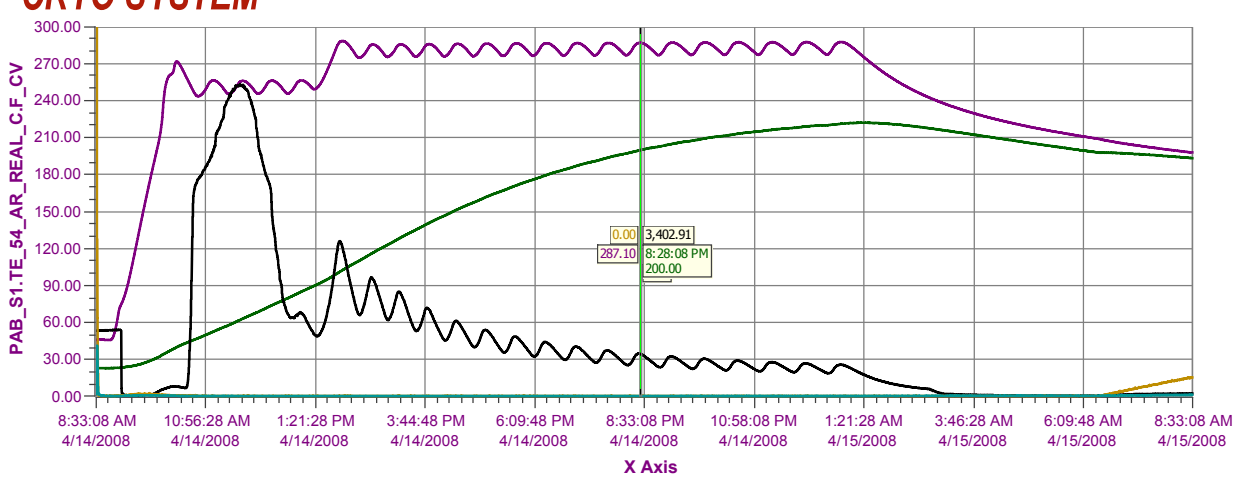

Pen Name	Description	Value	Eng Units	High Over ...	Low Over ...
PAB_S1.TE_56_AR_REAL_C.F_CV	O2 filter preheater temperature C (F_CV)	200	C	222	23
PAB_S1.TE_54_AR_REAL_C.F...	**O2 filter internal temperature C (...**	**287**	**C**	**289**	**46**
PAB_S1.AE_151_HAR_REAL_PP...	O2 Filter Near Dewpoint Meter ppm (F_...	3,402.9	ppm v/v	25,362.5	14.3
PAB_S1.PT_15_V_REAL.F_CV	LAr Transfer Line Insulating Vacuum	0.0001	Torr	1.0929	0.0001
PAB_S1.PT_154_V_REAL.F_CV	O2 Filter Cryostat Insulating Vacuum	0.0001	Torr	0.4112	0.0001

4/14/2008 8:33:08 AM | 24 Hours Ago | Current | 4/15/2008 8:33:08 AM