


DUNE Fiber glass (field cage support) 4/21/2016 – 4/25/2016

1. Liquid Test
2. The water peak observed at 4/23/2016 1:53 pm is due to a switch valve on the water measurer input. In fact, we do not observe a lifetime decreasing in correspondence of peak. The water content increasing is from 3 ppb to 7 ppb.

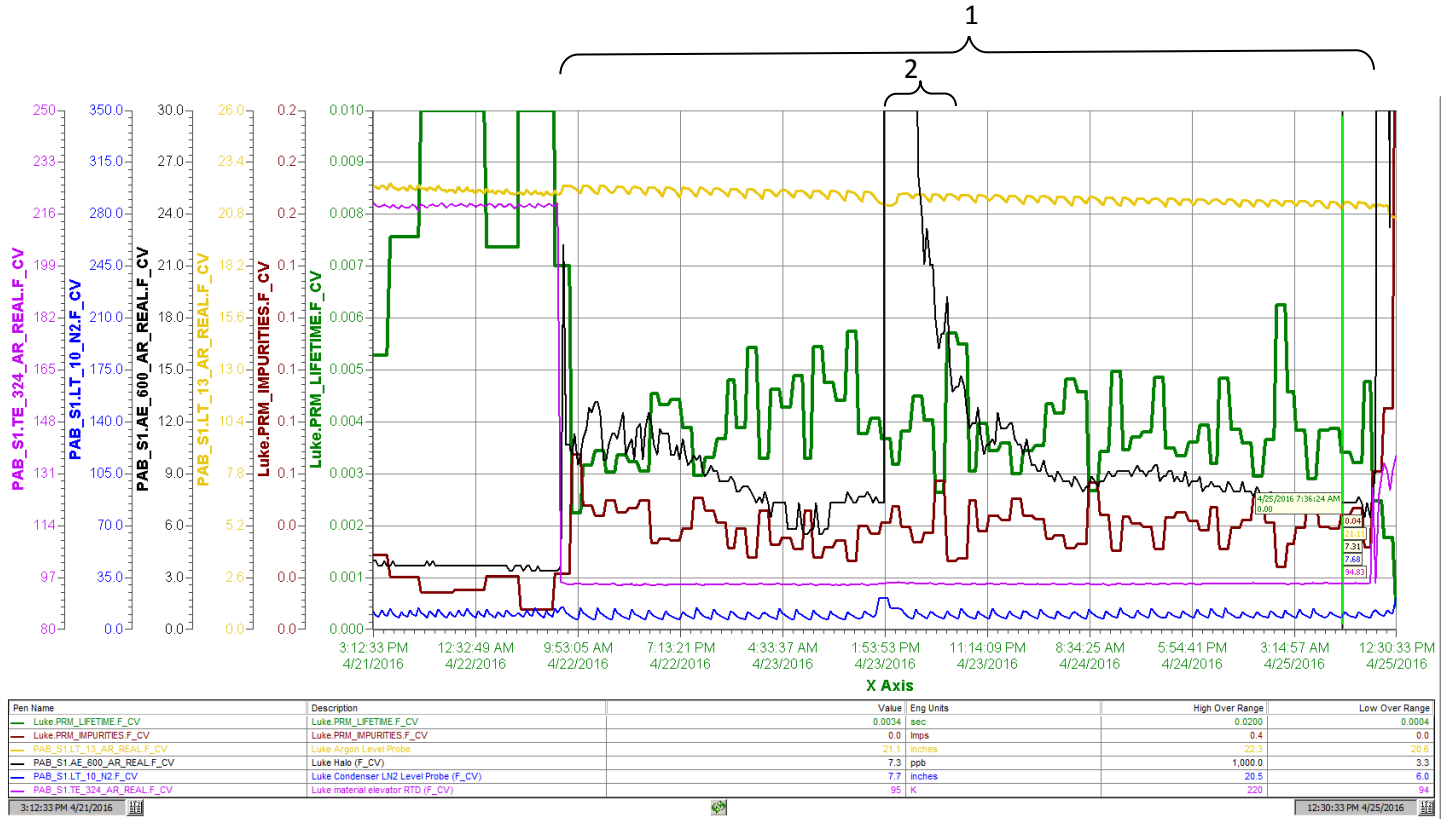

Lifetime – green pen

Impurities – brown pen

Liquid level – yellow pen

Water – black pen

Temperature – magenta pen