


Kemet Capacitors PHE 450 Test 3/1/2013 – 3/12/2013

1. Liquid test.
2. Zero test.

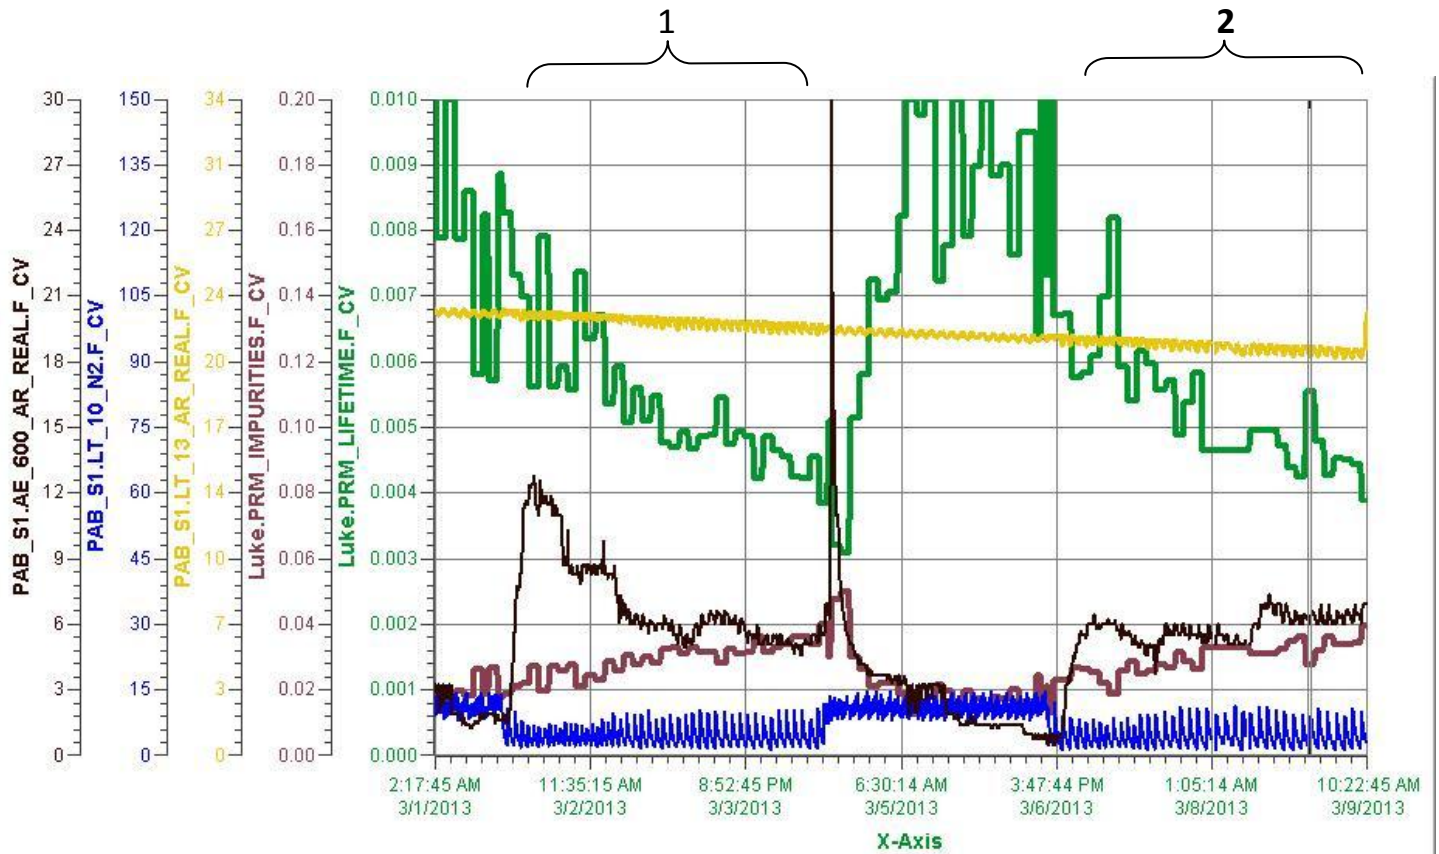

Pen Name	Description	Value	Eng Units	High Over Range	Low Over Range
— Luke.PRM_LIFETIME.F_CV	Luke.PRM_LIFETIME.F_CV	0.00550	sec	0.01218	0.00305
— Luke.PRM_IMPURITIES.F_CV	Luke.PRM_IMPURITIES.F_CV	0.0272	imps	0.0492	0.0123
— PAB_S1.LT_13_AR_REAL...	Luke Argon Level Probe	20.8	inches	23.1	20.5
— PAB_S1.LT_10_N2.F_CV	Luke Condenser LN2 Level Prob...	1.6	inches	14.6	0.9
— PAB_S1.AE_600_AR_REA...	Luke Halo (F_CV)	6.1	ppb	35.2	0.4

3/1/2013 2:17:45 AM 3/9/2013 10:22:45 AM