


PVC cable

Test 2 (no evacuation of the cable)

Room temperature test.

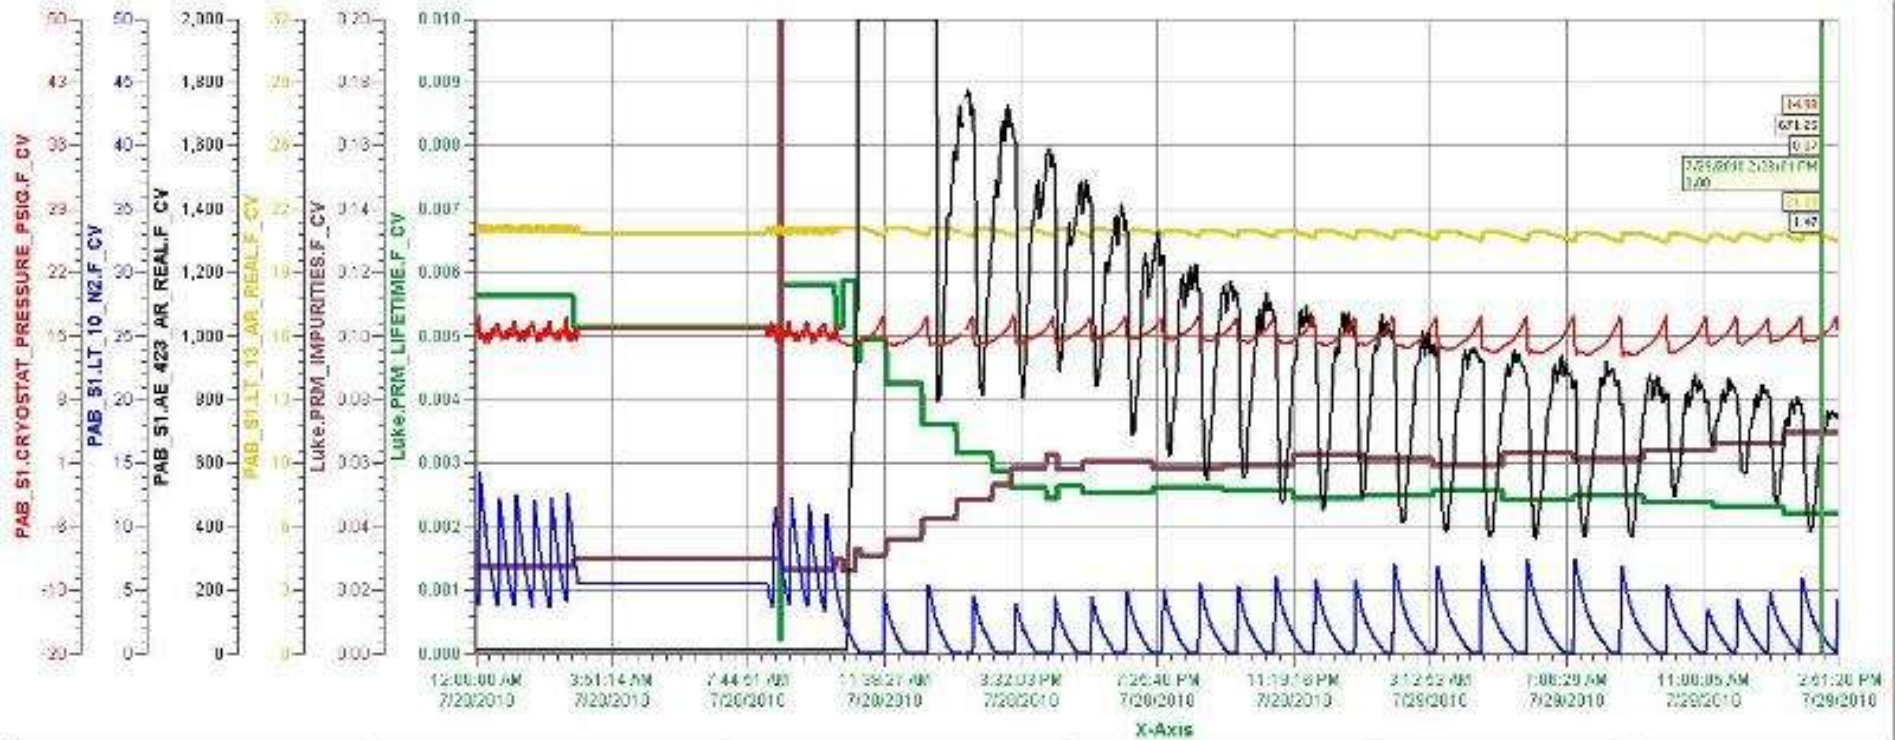

Pen Name	Description	Value	Eng Units	High Over Range	Low Over Range
— Luke.PRM_LIFETIME.F_CV	Luke.PRM_LIFETIME.F_CV	0.00218	sec	0.00583	0.00018
— Luke.PRM_IMPURITIES.F_CV	Luke.PRM_IMPURITIES.F_CV	0.0889	frps	0.9220	0.0257
— PAB_51_LT_13_AR_REAL.F_CV	Luke Argon Level Probe	21.1	inches	21.0	20.7
— PAB_51_AE_423_AR_REAL.F_CV	HALO H2O meter (F_CV)	671.3	ppb	3,000.0	3.4
— PAB_51_LT_10_N2.F_CV	Luke Condenser LN2 Level Probe (F_CV)	1.5	inches	14.3	-0.0
— PAB_51_CRYOSTAT_PRESSURE.PSI	Luke Vapor Pressure	15.0	psig	17.3	12.8

7/29/2010 12:00:00 AM Start of Yesterday Current 7/29/2010 2:01:30 PM