



Polymide Ring Spacers w/silicone Adhesive – PSL_007

15/Jun/2016 – 16/Jun/2016

<i>PAB Materials Test System</i>	
Date of Receipt	16/JUN/16 , logbook entry # 5265
Sample Name/Description	Polymide Ring Spacers w/silicone Adhesive PSL_007
Sample	
Composition:	Electronic board
Picture Location:	data base
Weight:	60.7 g
Dimensions/Area:	length approx. 123 mm, width 77 mm
Source:	Jonathan Heise, University of Wisconsin-Madison
Preparation:	dry clean
Submerging in LAr or LH2	x
Time in the airlock(hrs)	
Vacuum:	
Purge	22 hours with gas Argon from Luke
Liquid Test	
Start Time/Date, End Time/Date :	15/JUN/2016 8:30 AM, 16/JUN/2016 8:00 AM
PrM run # :	28265
Condenser state:	on
Filter state/settings:	off
H2O reading:	increased from 3.0 to 6.6 ppb
Temperature:	95 K
Liquid Level	21.2 inches
Lifetime:	7-8 ms

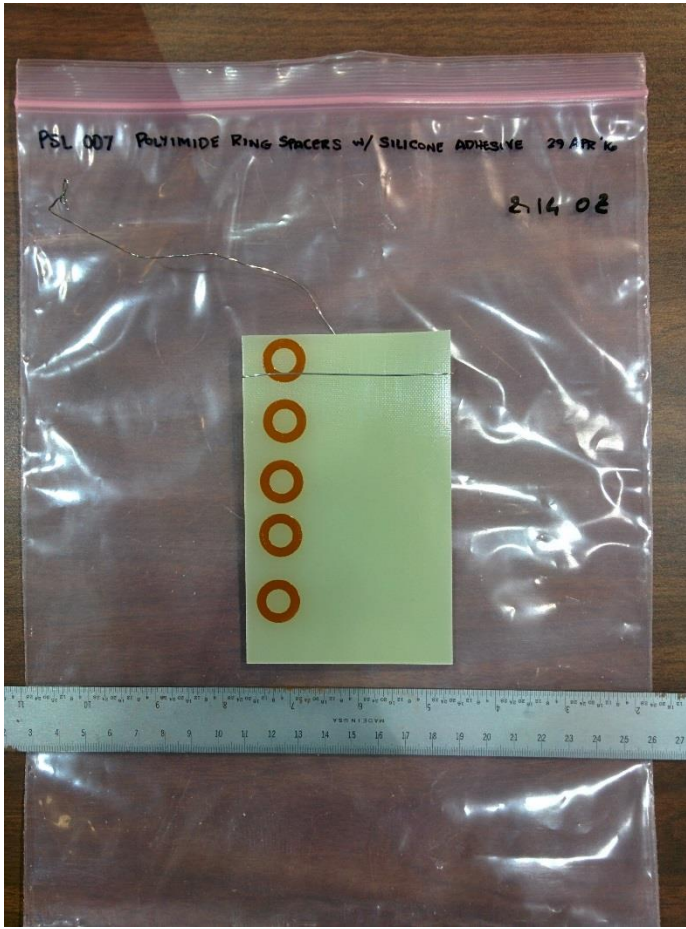

1. Liquid Test

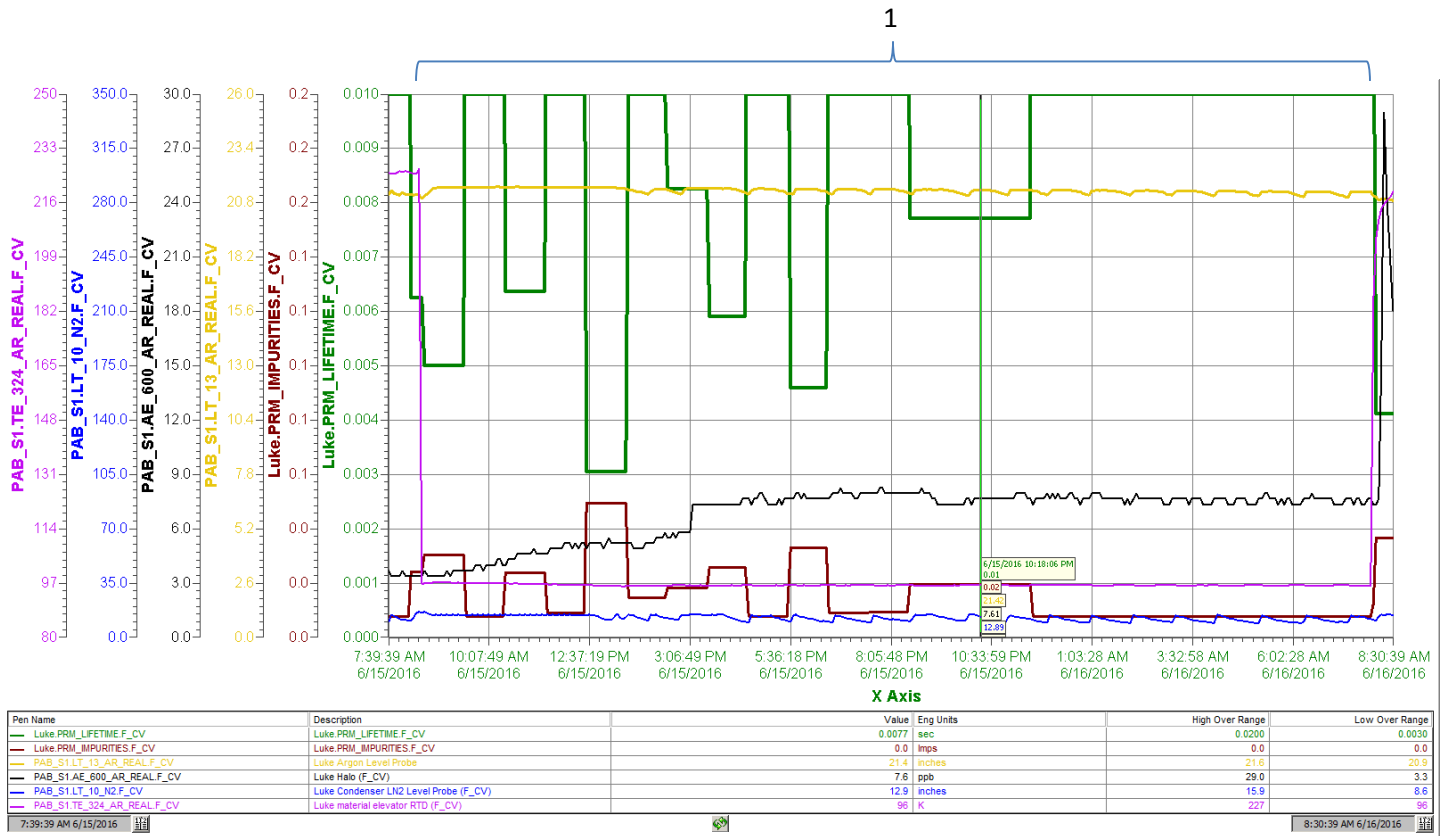

Lifetime – green pen

Impurities – brown pen

Liquid level – yellow pen

Water – black pen

Temperature – magenta pen