



SHV Connector Test 10/26/2010 – 11/8/2010

Room temperature test.

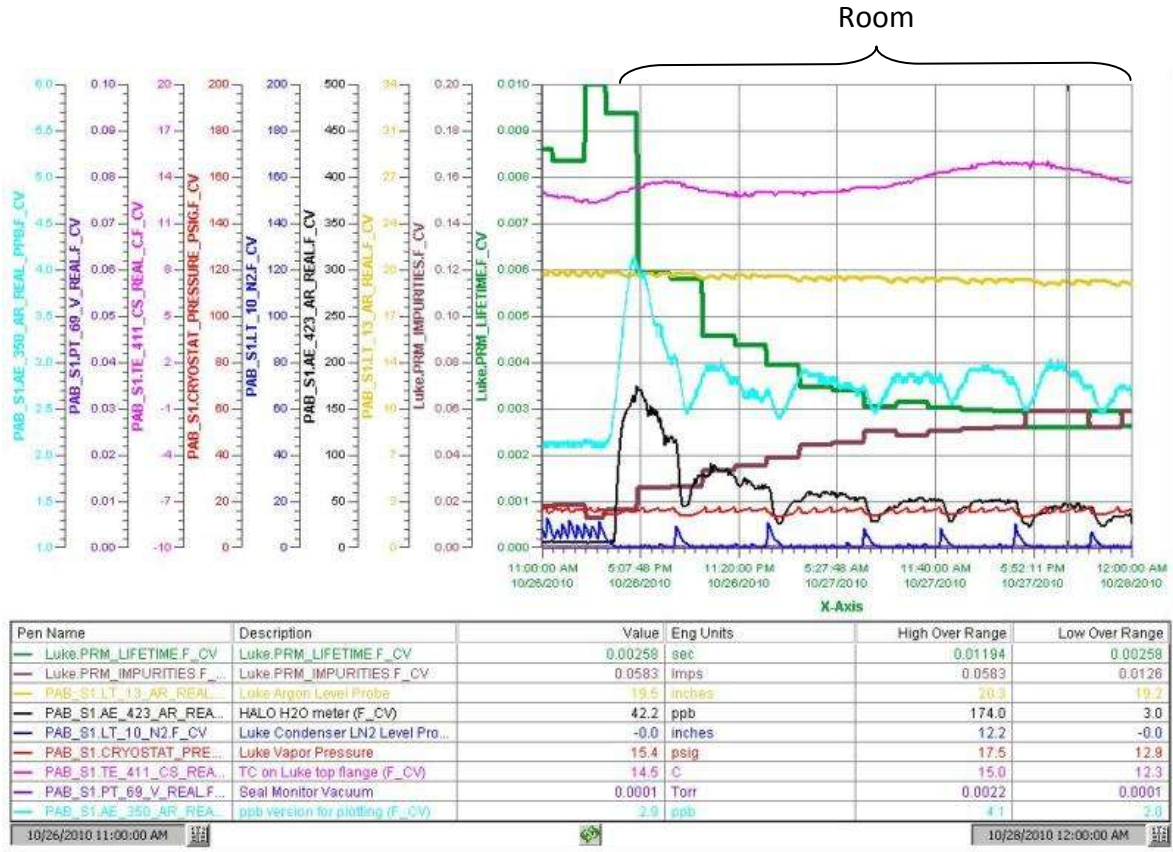


Vapor test and Liquid test.

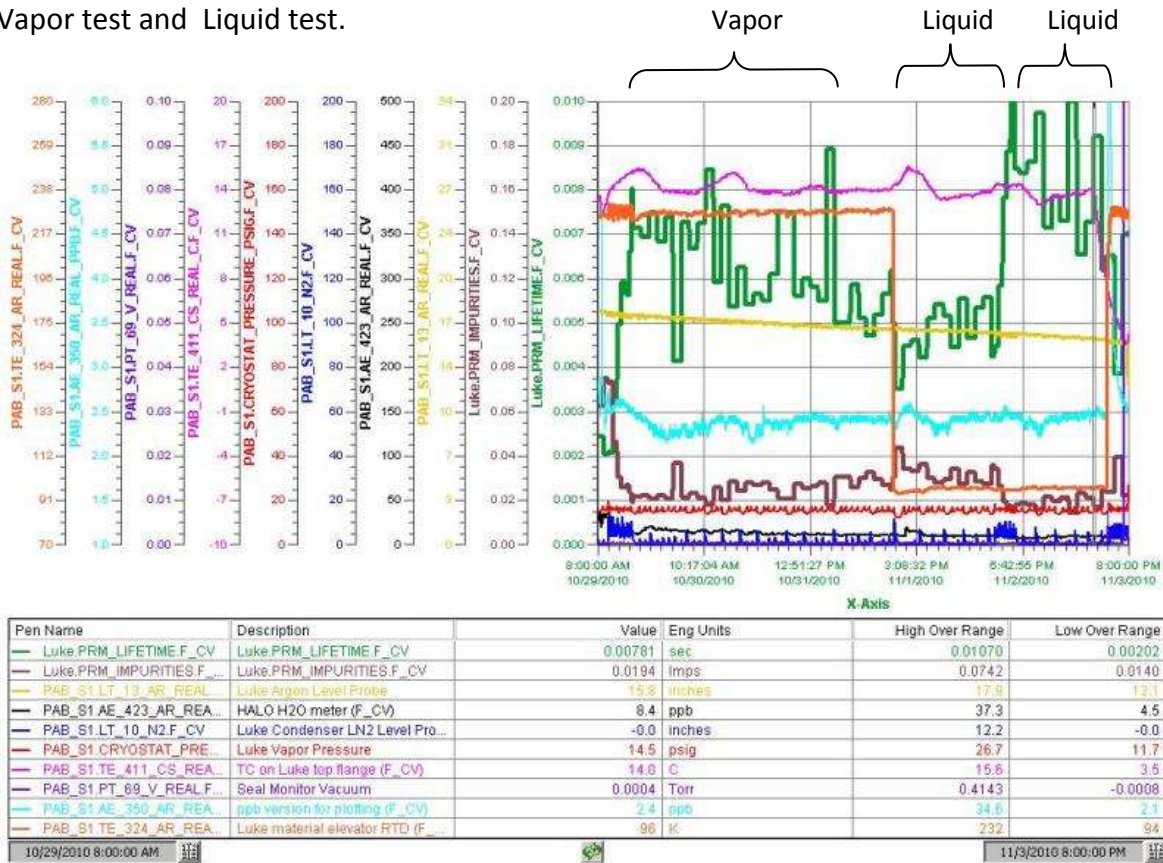

Zero test.

Zero

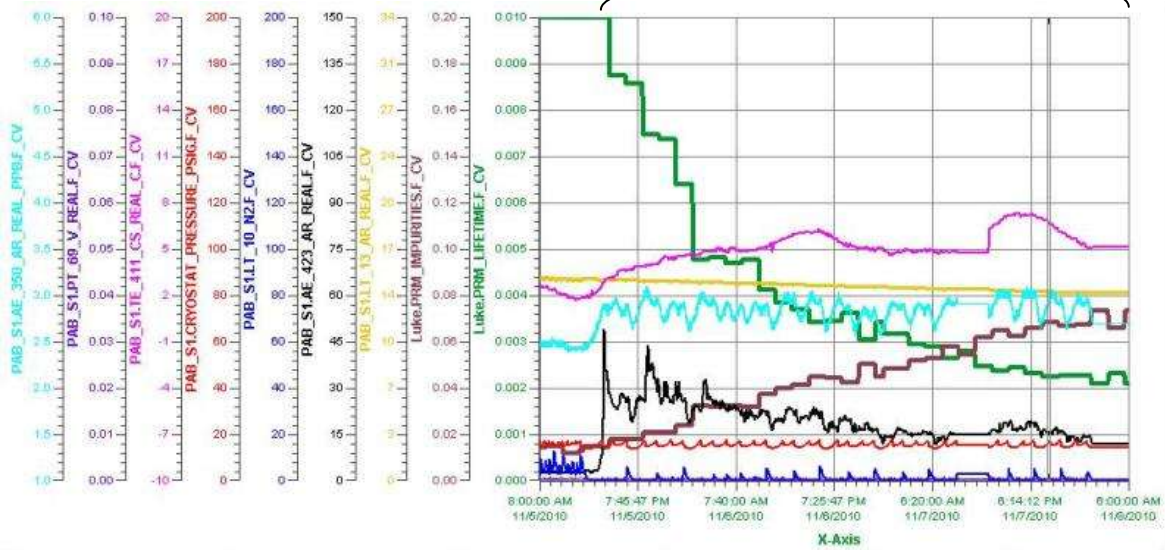

Pen Name	Description	Value	Eng Units	High Over Range	Low Over Range
Luke.PRM_LIFETIME_F_CV	Luke.PRM_LIFETIME F_CV	0.00222	sec	0.01330	0.00206
Luke.PRM_IMPURITIES_F_CV	Luke.PRM_IMPURITIES F_CV	0.0678	Imps	0.0728	0.0113
PAB_S1_LT_13_AR_REAL	Luke Argon Level Probe	13.6	inches	14.9	13.7
PAB_S1_AE_423_AR_REAL	HALO H2O meter (F_CV)	15.2	ppb	48.8	2.3
PAB_S1_LT_10_N2_F_CV	Luke Condenser LN2 Level Pro...	-0.0	inches	12.3	-0.0
PAB_S1_CRYOSTAT_PRE	Luke Vapor Pressure	15.8	psig	17.2	13.3
PAB_S1_TE_411_CS_REAL	TC on Luke top flange (F_CV)	6.7	C	7.3	1.6
PAB_S1_PT_69_V_REAL_F_CV	Seal Monitor Vacuum	0.0001	Torr	0.0007	0.0001
PAB_S1_AE_350_AR_REAL	ppb version for plotting (F_CV)	2.9	ppb	3.1	2.4

11/5/2010 8:00:00 AM 11/8/2010 6:00:00 AM