


Teflon Cable Test 1/9/2010 – 1/22/2010

1. Room temperature test.
2. Liquid test.
3. Vapor test.
4. Zero test.

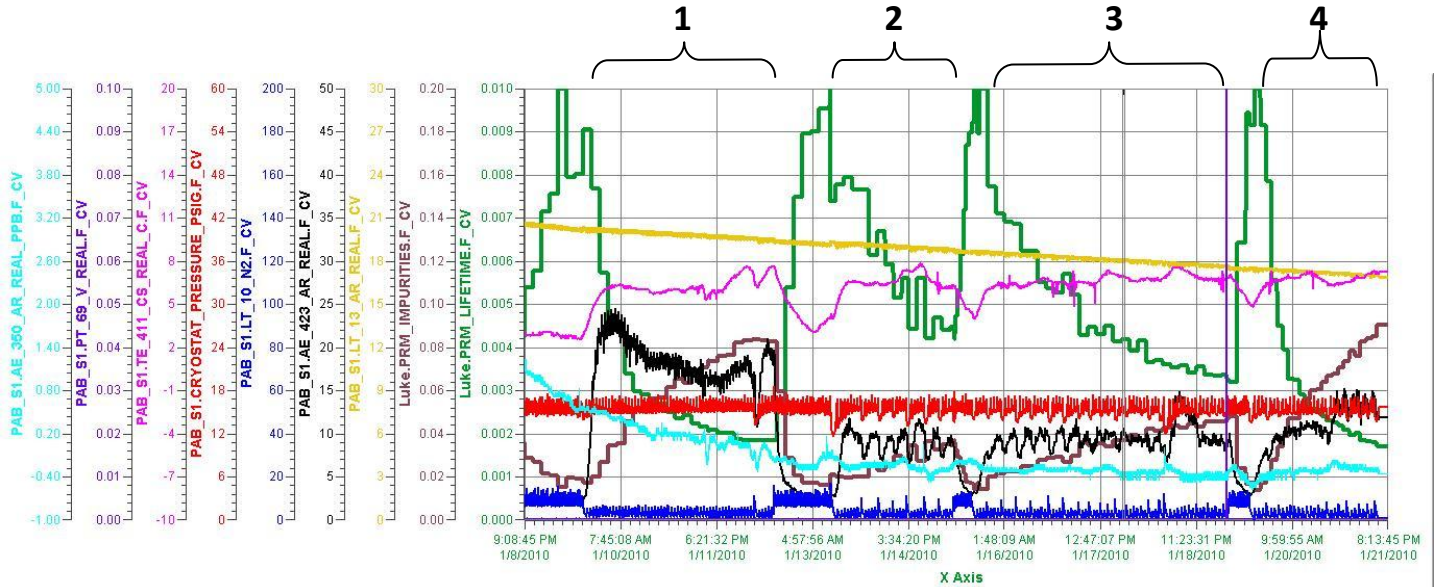

Pen Name	Description	Value	Eng Units	High Over Range	Low Over Range
— Luke.PRM_LIFETIME.F_CV	Luke.PRM_LIFETIME.F_CV	0.00415	sec	0.01142	0.00168
— Luke.PRM_IMPURITIES.F_CV	Luke.PRM_IMPURITIES.F_CV	0.0362	lmps	0.0895	0.0131
— PAB_S1_LT_13_AR_REALF_CV	Luke Argon Level Probe	18.1	inches	20.7	16.8
— PAB_S1_AE_423_AR_REALF_CV	HALO H2O meter (F_CV)	10.0	ppb	24.5	2.1
— PAB_S1_LT_10_N2_F_CV	Luke Condenser LN2 Level Probe (F_CV)	3.6	inches	18.6	-0.0
— PAB_S1_CRYOSTAT_PRESSURE_PSI...	Luke Vapor Pressure	14.8	psig	18.6	11.6
— PAB_S1_TE_411_CS_REAL_C_F_CV	TC on Luke top flange (F_CV)	6.9	C	7.9	2.5
— PAB_S1_PT_69_V_REALF_CV	Seal Monitor Vacuum	0.0001	Torr	5.7104	0.0001
— PAB_S1_AE_360_AR_REAL_PPBF_CV	ppb version for plotting (F_CV)	-0	ppb	1	-1

1/8/2010 9:08:45 PM

1/21/2010 8:13:45 PM